



Bionova® MiniPro Auto-reader

for Hygiene Monitoring Systems

R12 | 12.2025

WARNING: This product contains dry natural rubber.



Index

4 Composition

- 4 Product description
- 4 Indications for use
- 4 Features

5 Safety information

- 5 Symbols
- 6 Operating conditions
- 6 Power supply specifications
- 6 Environment operating conditions

7 Product Compatibility and Incubation programs

- 7 The Bionova® MiniPro Auto-reader Incubation Program

7 Instructions for use

- 7 Start-up
- 9 Interpretation of results of PRO1 indicators
- 11 Disposal
- 11 Reprinting of results
- 11 Remaining incubation time
- 11 Audible alarm
- 11 Cancel reading
- 11 Temperature monitoring
- 12 Thermal paper specifications
- 12 Paper roll replacement
- 12 Set-up Mode
- 13 Time setting mode

13 Additional features

- 13 Firmware update

13 Bionova® Cloud Environment

- 14 Threshold Mode selection for PRO1 Indicators
- 14 ISO 15883-5 Threshold Mode
- 14 ISO 15883-5 Workflow
- 15 Bionova® Cloud Surface Eye Mobile App advanced features

15 Cleaning and maintenance

- 15 Cleaning and decontamination of external surfaces




16 Troubleshooting

- 16 Maintenance

17 Warranty

- 17 Term
- 17 Limitation of liability
- 17 Technical assistance

■ Composition

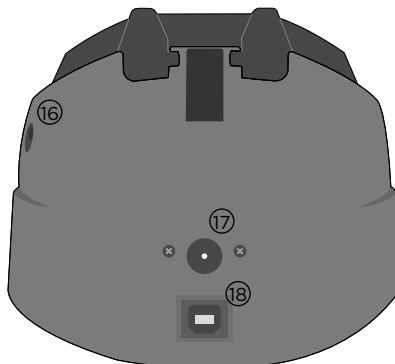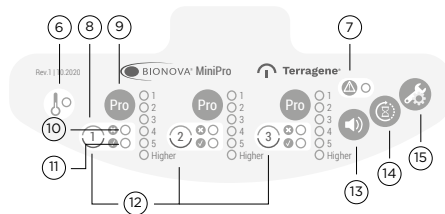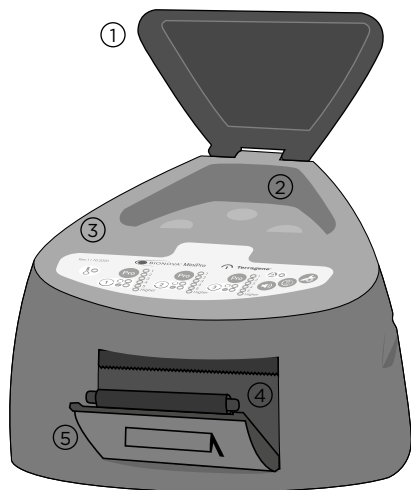

Product description

The Bionova® MiniPro Auto-reader was designed for the automatic readout of Terragene® Chemdye® Hygiene Monitoring System PRO1 Indicators (PRO1 Protein Pen Indicators) appropriate for the detection and quantification of surface proteins.

The Bionova® MiniPro Auto-reader incubates at 60 °C and performs a quantitative analysis over the Chemdye® PRO1 Protein Pen Indicators, adjusted by a BSA (Bovine Serum Albumin) reference curve. The Bionova® MiniPro allows the incubation and readout of three independent Chemdye® PRO1 Indicators simultaneously.

The Bionova® MiniPro Auto-Reader quantitative analysis has a detection limit of 0.5 µg and a quantification range from 1 to 50 µg of equivalent BSA Protein. The results are indicated with a resolution of 0.1 µg, with an accuracy greater than 90 % in the whole quantification range (CI95 %).

The Bionova® MiniPro Auto-reader also provides a printed ticket each time an automatic readout is completed for recording the results. This allows for easy result management, for documentation compliance and safekeeping.

Note: Do not place a new Protein Pen until the temperature is stable and the Temperature stability indicator stops blinking.

Indications for use

The Bionova® MiniPro Auto-reader incubates at 60 °C and reads the Terragene® Chemdye® Hygiene Monitoring System Indicators at the times prescribed in the User Manual.







Features

- ① Protective cover
- ② Incubation area
- ③ Control panel
- ④ Cavity for paper
- ⑤ Thermal printer
- ⑥ Temperature stability indicator
- ⑦ Blue attention light

- ⑧ Incubation position
- ⑨ Start incubation program button / Time left
- ⑩ Red LED indicator / Protein level above Threshold (HTM01- 01 Threshold mode) / Protein level above 1µg (ISO 15883-5 Threshold mode)
- ⑪ Green LED indicator / Protein level below Threshold (HTM01- 01 Threshold mode) / Protein level below 1µg (ISO 15883-5 Threshold mode)
- ⑫ Quantitative protein level LED indicators
- ⑬ Alarm cancellation button
- ⑭ Reprint of results
- ⑮ Configuration / Paper traction button
- ⑯ Hole for external temperature control
- ⑰ Socket for power supply plug (12 Volts DC)
- ⑱ USB port

■ Safety information

Symbols

-  **Humidity limitation.** Indicates the range of humidity to which the medical device can be safely exposed.
-  **Temperature limit.** Indicates the temperature limits to which the medical device can be safely exposed.
-  **Caution.** Indicates that caution is necessary when operating the device or control close to where the symbol is placed, or that the current situation needs operator awareness or operator action in order to avoid undesirable consequences.
-  **Caution, hot surface.** To indicate product can be hot and should not be touched without taking care.
-  **Consult instructions for use or consult electronic instructions for use.** Indicates the need for the user to consult the instructions for use.
-  **CE mark.** Indicates the product conforms to all legal requirements to be sold within the European Union/European Economic Area (EU/EEA).



Fragile, handle with care. Indicates a medical device that can be broken or damaged if not handled carefully.



Direct current. To indicate on the rating plate that the equipment is suitable for direct current only to identify relevant terminals.



For indoor use only. Indicates medical device be used indoors.



Keep away from sunlight. Indicates a medical device that needs protection from light sources.



Batch code. Indicates the manufacturer's batch code so that the batch or lot can be identified.



Manufacturer. Indicates the medical device manufacturer.



Date of manufacture. Indicates the date when the medical device was manufactured. This shall be expressed in accordance with ISO 8601-1 [year-month-day].



Serial number. Indicates the manufacturer's serial number so that the specific medical device can be identified.



Recycle electronic equipment. DO NOT throw this unit into a municipal trash bin when this unit has reached the end of its lifetime. Please recycle.



Keep dry. Indicates a medical device that needs to be protected from moisture.



This way up. To indicate correct upright position of the transport package.



Do not stack. Indicates product should not be stacked or top loaded.



Recyclable. Indicates that the marked item or its material is part of a recovery or recycling process.



Class II equipment. To identify equipment meeting the safety requirements for Class II equipment according to IEC 61140.



Contains or presence of natural rubber latex. Indicates the presence of natural rubber or dry natural rubber latex as a material of construction within the medical or the packaging of a medical device.



Polarity of d.c. power connector. To identify the positive and negative connections (the polarity) of a d.c. power supply, or the positive and negative connections on a piece of equipment to which a d.c. power supply may be connected.



To avoid risks and/or damaging the device:

- Use indoors only.
- Do not place the auto-reader in a room exposed to direct sunlight or to high luminous intensity lamps.

Safety information

- Do not place the auto-reader near devices that emit strong electromagnetic fields.
- Do not use the auto-reader on sloping surfaces or on surfaces that might be knocked, that may vibrate, be exposed to high temperatures, or high relative humidity.
- Disconnect the power cord before cleaning.
- Do not use abrasive, corrosive cleaners or disinfectants.
- Do not immerse into any liquid. Do not pour liquid into it.
- Make sure the auto-reader is connected to an appropriate electrical mains outlet socket.
- Use only the included power supply (AC power adapter), power supply's AC plug, power supply cords, and USB cable. Check that all items included are in good condition every day. If any of them is damaged, stop using them. The use of cables, adapters, cords, and/or power supplies different from the ones included may cause fires, electrical shocks, or even physical injuries.
- Do not plug any devices into the auto-reader's USB port other than a personal computer (PC). The PC must be compliant with IEC 60950-1, IEC 62368-1 or comparable, with safety extra-low voltages on its USB ports. Ask a qualified technician to check that the device is compatible. Attaching any other device to the USB port may damage the auto-reader and may not be safe for the user.
- Do not attempt to repair the auto-reader yourself. This could lead to major and irreversible damages to the device. If the auto-reader malfunctions, contact your local distributor for further assistance.



To reduce the risks associated with contaminated surfaces with protein levels outside the user-defined threshold:

- Please read, understand, and follow the Instructions for Use of each Protein Pen before its incubation.
- Do not remove the Protein Pen before the auto-reader reports the final readout result. Check the printed ticket.



To avoid a potentially hazardous situation:

- Avoid contact with the hot metal block inside each incubation position.
- Do not insert your fingers, or any other element, into the incubation positions.
- Place only compatible indicators inside the incubation positions.

Note: Do not use this product other than in the manner specified by Terragene S.A., otherwise the protection provided by the product might be affected.

Note: Only Terragene S.A. authorized personnel may access or service the internal components of the auto-reader. Parts

or components inside the auto-reader should not be handled by the user.

Operating conditions

Power supply specifications

Input parameters	Operating conditions	Units
Voltage range	(100-240)	AC Volts
Frequency	50/60	Hertz
*Current	0,5	Amperes

Output parameters	Values	Units
Voltage	12	DC Volts
**Current	2	Amperes

* 1 Ampere in USA and Canada.

** 3 Amperes in USA and Canada.

Terragene S.A. recommends the use of Uninterruptible Power Supply (UPS) instead of voltage stabilizers since they fulfill two functions: To stabilize and maintain the energy during a power outage.

Environment operating conditions

Environmental conditions	Operating conditions	Units
Altitude	3500 (max.)	Meters
Operation temperature	10-30	Celsius
Relative humidity	30-80	%
Installation/Over-voltage	Category II	
Pollution degree	2	
Storage temperature	5-40	Celsius
Voltage	12	DC Volts

Device safety compliance

The Bionova® MiniPro Auto-reader complies with the following standards and directives:

Electrical Safety	IEC 61010-1 IEC 61010-2-010 Low Voltage Directive 2014/35/EU
Electromagnetic Compatibility (EMC)	EN 61326-1 EMC Directive 2014/30/EU
European Commission	RoHS Directive 2011/65/EU WEEE Directive 2012/19/EU

The Bionova® MiniPro Auto-reader does not represent photobiological risk and does not generate dangerous optical radiation if used within normal operation conditions as per the

Safety information

requirements of IEC 62471 Standard.
Designed under Quality Management System standards
ISO 13485:2016/ EN ISO 13485:2016.

■ Product Compatibility and Incubation programs

The Bionova® MiniPro Auto-reader Incubation Program

The following incubation program is available for your auto-reader.

Temperature selection	Time selection	Incubation program
60 °C	PRO (4 min)	PRO at 60 °C

Follow the Protein Pen Instructions for Use before its incubation.

■ Instructions for use

Note: Remember to set the auto-reader local date and time before starting incubations.

Start-up

1Place the Bionova® MiniPro Auto-reader on a firm surface, free from vibrations, away from direct sunlight, hot or cold air flows, chemical, corrosive or flammable substances. Do not place the auto-reader in a way that makes disconnecting the power supply's AC plug from the mains difficult. Leave a space of at least 10 cm from the auto-reader to the closest wall. Do not move the auto-reader periodically or during its use. Connect the auto-reader to a secure and stable electrical mains outlet socket.

Note: Do not wet or heat the device. If liquid is spilled on the auto-reader, disconnect it and clean it. For more information, please refer to the following section: *Cleaning and maintenance*.

2Switch on your auto-reader by connecting the power supply's AC plug to the mains and then connect the plug at the other end of power supply to the rear of the auto-reader.

Note: Before turning it on, verify that all reading positions are empty.

Note: If the Blue attention light starts blinking after switching on the auto-reader, check that the printer's door is tightly closed and that the printer has paper. For more information, please refer to the following section: *Replacement of the Paper Roll*.

3Set the auto-reader local date and time. For more information, please refer to the following section: *Time setting mode*.

All devices are manufactured with the following settings:

- Time zone: UTC +0:00
- Printing language: English

If you want to change the time zone, or the printing language, please refer to the following section: *Modification of time zone, Modification of printing language*.

4Select your preferred Protein Quantification Threshold Mode for your auto-reader from the two Threshold modes available: Threshold based on HTM 01-01 Standard or Threshold based on ISO 15883-5:2021 standard.

Note: The ISO 15883-5:2021 Threshold Mode is available exclusively for the Chemdye® PRO1 MICRO indicator.

For the selection of a Threshold mode and a Threshold value, please follow the indications detailed in the *Threshold Mode Selection* section on the *Bionova® Cloud Environment* section.

All devices are manufactured with the following settings:

- Default Threshold Mode: HTM 01-01
- Default Protein Threshold: 1 µg

Make sure that the selected Protein Quantification Threshold Mode is in accordance with your specifications before performing an incubation. The Threshold Mode cannot be changed during ongoing readings.

5Wait until the Temperature stability indicator stops blinking, indicating that the auto-reader has reached a steady working temperature.

Note: Do not place an indicator on an incubation position before the incubation temperature is stable.

6Once the Temperature stability indicator remains stable, a one-time automated test to check each position internal status will be carried out (auto-test).

Once the auto-test has been completed, the Green LED indicator will turn on to indicate that the position can be used to perform readings. Otherwise, the Red LED indicator will turn on to indicate that an error has occurred.

When the auto-reader detects an error in a position, the position will be disabled to guarantee the reliability of the results and no further readings will be possible.

To indicate that a position has been disabled, the Red LED indicator will blink indefinitely.

⤵ Instructions for use

Note: To ensure the auto-test works properly, keep the protective cover closed when the auto-test is running.

7| Once the auto-test has been completed, the readings can be initiated on any incubation position if the position has not been disabled. Place a Chemdye® PRO1 indicator in an incubation position to start an incubation. Press and hold the button of the chosen position for 1 second to enable the position's readout mode. The auto-reader will emit a short beeping sound and the 1 µg quantitative protein level led indicator will blink for a moment. After that, two short beeping sounds will be emitted indicating that the incubation position is enabled and ready to start an incubation.

An incubation position cannot be enabled before the incubation temperature is stable and the auto-test has been carried out successfully. Please wait until both processes are completed before placing an indicator on an incubation position.

8| Use a compatible Chemdye® PRO1 indicator to take a sample from the surface to be analyzed. Make sure to follow the indicator's Instructions for Use while taking the sample. A summary of the swabbing process is also detailed on Figure 1.

9| After a sample from the desired surface has been taken, place the Chemdye® PRO1 indicator into the enabled incubation position. Insert the indicator fully inside the incubation position, as shown on the auto-reader's label. When the indicator is in the correct position, the indicator cannot be rotated. (Figure 2).

Note: Make sure that the solution is correctly mixed and the reading cone has a sufficient amount of solution before starting an incubation.

Note: Make sure that the indicator's swab is not inside the reading cone before starting an incubation.

10| Once the indicator is placed on the incubation position, press and hold the **Pro** button for 1 second to start the incubation and readout process. Once the process starts, the Red and Green LED indicators will start to blink and will keep blinking throughout the whole incubation and readout process. Wait until the incubation and readout process is completed before removing the indicator.

Note: Do not move or remove or change the indicator placement once a reading process has begun, as it could lead to errors in the incubation and/or readout process.

11| Once the incubation and readout process is completed, the Red and Green LED indicators will stop blinking and the auto-reader will indicate the quantity of protein in µg found in the

sample by turning on the corresponding Quantitative protein level LED indicator. A ticket will also be printed detailing the protein quantity along with other useful information related to the readout process.


The protein quantity found on the sample is also used to obtain and inform a readout result depending on the Protein Quantification Threshold Mode and threshold values selected on your auto-reader. For more information, please refer to the section: **Interpretation of results of Protein Pen indicators**. After a Readout result is informed remove the indicator from the incubation position and press the: **Pro** button once to reset the incubation position to its stand-by state.

Note: The color of the solution in the Chemdye® PRO1 indicator can be used for a qualitative reading only if the pen is removed immediately when the incubation program ends. An audible alarm will sound 30 seconds before the program finishes to alert the operator that completion is near. If the protein pen is not removed promptly after the result is indicated, the solution color will continue to change.


12| To save the printed ticket, pull upward for the paper to be cut with the serrated edge of the printer.

Note: If there is no paper for ticket printing, the Blue attention light will start blinking. For more information on how to change the paper roll refer to section: **Replacement of the paper roll**. After the paper has been replaced, you can reprint the last 3 readout results following the **Reprinting of Results** section instructions.

Figure 1




Remove swab and add the moisturizer




Swab the desired surface by applying a strong pressure


Instructions for use




Place the swab back into the device




Activate




Shake downwards vigorously until the solution turns to green and reaches the readout cone reference volume




Shake for 15 seconds with the swab inside the readout cone




Slide swab upwards without completely removing



Again, shake downwards vigorously and reach the readout cone reference volume




Readout cone without swab



Incubate immediately and read

Figure 2



Insert the pen on the incubation/reading position

Interpretation of results of PRO1 indicators

Once a PRO1 Indicator readout process is finished, the auto-reader will inform the equivalent μg of protein quantity found on the sample using a BSA (Bovine Serum Albumin) calibration curve through the Quantitative Protein Level LED Indicators and through a printed ticket.

The protein quantity found on the sample is also used to obtain and inform a readout result depending on the

⬇ Instructions for use

Threshold mode and threshold values selected on your auto-reader. Such readout result can be either Positive or Negative for HTM 01-01 Threshold Mode, or Negative, Alert, or Action for ISO 15883-5 Threshold Mode.

Note: To select a Threshold mode and its values please refer to the *Threshold Mode selection on Bionova® Cloud Environment* section.


Readout results for HTM01-01 Threshold Mode

HTM 01-01 Threshold Mode is the default Protein Quantification Threshold mode of your auto-reader.

HTM 01-01 guidelines indicate the use of a single protein quantity threshold to evaluate cleaning efficacy. The guidelines recommend that the residual protein level upper limit of acceptable protein contamination after processing is 5 µg BSA equivalent per instrument side, indicating as well that lower levels may be recommended for particular applications.

Note: Refer to the HTM 01-01 guidelines for detailed information on how to implement the standard to your processes.


If HTM 01-01 Threshold Mode is selected as the readout threshold mode on your auto-reader, each time a readout is completed the protein quantity will be informed through the Quantitative Protein Level LED Indicators and a printed ticket:

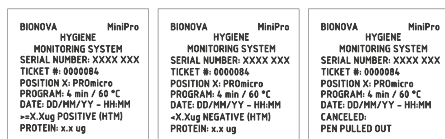

POSITIVE

NEGATIVE

CANCELED



Approximate amounts of BSA expressed in µg.

If the protein quantity detected on the sample is lower than the selected threshold, a negative readout result will be informed and the auto-reader will turn on the Green LED indicator. If the quantity detected is greater than the selected threshold, a positive readout result will be informed and the auto-reader

will turn on the Red LED indicator. The readout result will be detailed on the printed ticket as well. Furthermore, if the auto-reader is connected to the Bionova® Cloud Environment, the readout results can be found on the *Hygiene Monitoring > Finished web page of Bionova® Cloud Web interface*.

Take action immediately whenever a POSITIVE Readout Result is informed as this indicates that the protein quantity found does not comply with the user defined quality standards set for the cleaning process.

Readout results for ISO 15883-5 Threshold Mode

The ISO 15883-5:2021 standard indicates the use of two different protein quantity thresholds to evaluate cleaning efficacy: An Action threshold, and an Alert threshold. ISO 15883-5 based thresholds are expressed as ratios in µg/cm2 units that relates protein quantity found in a sample (µg) and the swabbing surface (cm2) on which the sample was taken. According to the standard, each threshold has different implications:

Alert threshold: The alert levels are the target levels of cleaning efficacy that the cleaning process should achieve. Recommended threshold value 3 µg/cm2. Lower values may be recommended for particular applications.



Action threshold: The action levels are the maximum criteria for acceptable cleaning efficacy during testing of a sample. Recommended threshold value 6.4 µg/cm2. Lower values may be recommended for particular applications.

Values between the two thresholds should be investigated, but are considered to pass cleaning requirements described in ISO 15883-5:2021 standard.

Note: Refer to the ISO 15883-5:2021 standard for detailed information on how to implement the standard to your processes.

If ISO 15883-5 Threshold Mode is selected as the readout threshold mode on your auto-reader, each time a readout is completed the protein quantity will be informed by the auto-reader through the Quantitative Protein Level LED Indicators and through a printed ticket:

Instructions for use



Approximate amounts of BSA expressed in µg.

Also, as a quick visual cue of the protein quantity found on the sample, the device will turn on the Red LED Indicator if the protein quantity is above 1 µg, or the Green LED Indicator if the protein quantity is below 1 µg.

Note: Please keep in mind that according to ISO 15883-5:2021 standard the protein quantity found in a sample (in µg) needs to be related to the swabbed surface area to obtain a readout result (in µg/cm²) that can be comparable with the selected Alarm and Alert thresholds (also in µg/cm²).

Once the protein quantity in the sample has been obtained by the auto-reader, and the swabbed surface information has been obtained with the Bionova® App. The information is finally linked together by the Bionova® Cloud Environment to inform the readout result. Please refer to ISO 15883-5:2021 on *Bionova® Cloud Environment* section for a step by step guide to upload and link data on Bionova® Cloud Environment.

Once the data has been linked, the readout result will be shown on the *Hygiene Monitoring > Finished tab of Bionova® Cloud Web Interface*. Depending on the threshold values selected, the informed readout result can be as follows:

If the protein quantity found on the swabbed surface (µg/cm²) is below the Alert Threshold. The readout result will be informed as **NEGATIVE**.

If the protein quantity found on the swabbed surface (µg/cm²) is above the Alert Threshold but below the Action Threshold. The readout result will be informed as **ALERT**.

If the protein quantity found on the swabbed surface (µg/cm²) is above the Action Threshold. The readout result will be


informed as **ACTION**.

Take action immediately whenever an **ACTION** Readout Result is informed as this indicates that the protein quantity found does not comply with the user defined quality standards set for the cleaning process.

Disposal


Discard the PRO1 indicator according to your country's sanitary regulations. It is not possible to use or incubate a PRO1 indicator more than once. Please refer to the PRO1 indicator Instructions for Use.


Reprinting of results

The auto-reader allows reprinting of the last 3 results. For reprinting the results, press and hold for 3 seconds the button: .


Remaining incubation time

The auto-reader allows you to verify the remaining incubation time in every reading position by printing a ticket.



To check the remaining time in a single reading position, press and hold for 3 seconds the button: .

To check the remaining time on all reading positions, press and hold simultaneously and for 3 seconds two of the buttons: . In each case a ticket will be printed informing the remaining time as shown below.

Audible alarm

An audible alarm will sound every time a positive result is detected by the auto-reader. The alarm allows the user to immediately detect a positive result without the need to visually check the device. To cancel the alarm, press the button: .

Cancel reading

The user can cancel the reading of any of the 3 positions by simultaneously pressing and holding for 3 seconds the button:  of the chosen position and the following button: . Once a reading is canceled a ticket will be printed.

Temperature monitoring

The auto-reader features an automated internal temperature control. If the incubation temperature falls outside of the specified range of 60 ± 2 °C, the temperature stability indicator

⚡ Instructions for use

light will start to blink. The incubation temperature can be externally monitored by placing an external thermometer in the hole for external temperature control located at the back of the device.

Thermal paper specifications

Recommended paper: 73450 (order direct from ASP), JUJO AF50KSE3, or equivalent.

Paper width: 57 mm

Maximum paper thickness: 60 g/m²

Maximum diameter size: 23 mm

Paper roll replacement



1| To replace the paper roll, pull the handle on the printer door. Open the cover and remove the empty roll.



2| Place the new paper roll with the outer side up.



3| Close the printer cover by pressing on the sides of the lid.

Note: To advance the paper, press the button: ⚙️.

Set-up Mode

The auto-reader features a configuration mode that enables

you to set the printing language and the date format and time zone in the device.

To access the set-up mode, turn on the auto-reader while holding down the button: ⚙️. If the auto-reader has successfully entered the set-up mode, the Red and Green LED indicators in all incubation positions will turn on and a ticket will be printed. To change the date format, time zone and printing language, please follow the instructions listed below. To exit the set-up mode, turn off the device.

Modification of date format and time zone

The date format and time zone modification function allows changing the date format and time zone of the device to suit better the local characteristics of your country. To select the device's date format, make sure that the device is in set-up mode and press the button: ⚙️.

The current date format will be printed to set a reference value and the green LED indicator corresponding to incubation position 1 will start blinking. To move back and forth between the options available, press the buttons: ⏪ or ⏩. After 2 seconds, a ticket with the selected format will be printed to set a reference. Three types of date format are available: DD/MM/YY, MM/DD/YY and YY/MM/DD.

Note: The default date format is DD/MM/YY.

To save the selected date format, press and hold for 3 seconds the button: ⚙️ for 3 seconds.

To exit without saving the changes, turn off the device. Once the date format has been modified and saved, the auto-reader will enter the Time Zone Modification Mode automatically. The current date (with the previously selected format) and the current time will be printed to set a reference.

To subtract hours, press the button: ⏪.

To add hours, press the button: ⏩.

After 2 seconds, a ticket will be printed, informing the selected time zone. To confirm the change, press and hold for 3 seconds the button: ⚙️.




To discard the changes, turn off the device.

Note: The green LED indicator corresponding to incubation position 1 will stop blinking once both, the date format, and time zone modifications are saved.

Modification of printing language

This functionality allows changing the language that appears on the tickets. To select the device's printed ticket's language, make sure that the device is in set-up mode and press the button: ⏪.

Instructions for use

The current language and list of available languages will be printed to establish a reference. To move back and forth between the options available, press the buttons:  or . After 2 seconds, a ticket will be printed informing the selected language. To confirm the change, press and hold for 3 seconds the button: .

To discard the changes, turn off the device.

Time setting mode

Modification of the time using the firmware update utility

Connect the auto-reader via the USB port to a PC and run the Firmware Update Utility. Select the auto-reader and press the "Clock Sync" button, the auto-reader internal time and date will be synchronized with the PC's current time and date. Synchronization can only be done if there is not an ongoing reading.

Modification of the time using Bionova® Cloud Agent

Connect the auto-reader via the USB port to a PC and run Bionova® Cloud Agent. Select the auto-reader and press the "Clock Sync" button, the auto-reader internal time and date will be synchronized with the PC's current time and date. Synchronization can only be done if there is not an ongoing reading.

Additional features

Firmware update

The Bionova® MiniPro Auto-reader firmware can be updated (a program inside the auto-reader checks and defines the various features) with the Bionova® Bioupdate utility. The Bionova® Bioupdate connects to the Internet to check, download, and install the latest firmware version available for your auto-reader. The update process only lasts a few seconds and is carried out without the loss of any auto-reader's data.

Please visit www.terragene.com/software to download Bionova® Bioupdate.

Update process

Before updating the device, make sure that the Bionova® Cloud Agent is closed. Switch off the auto-reader for five

seconds, then switch the auto-reader back on and follow the next steps:

1 Using the included USB cable, connect your Bionova® MiniPro to a PC where Bionova® Bioupdate has been previously installed. Make sure the PC has a working Internet connection.

2 Run Bionova® Bioupdate.


3 Select the auto-reader from the list and press the button: **Start**.

4 Wait until the software indicates that update process has been completed. The auto-reader will print an update confirmation ticket. If it was already up to date, the ticket will not be printed.

Note: It is recommended that this process be carried out once a year unless required by the manufacturer.

Bionova® Cloud Environment

The new Bionova® Cloud environment is a Cloud based solution that integrates the information generated by Terragene® electronic devices with an easy-to-use Web App for the traceability of sterilization and disinfection control applications. The Bionova® Cloud environment is composed by two main components: The Bionova® Cloud Traceability Software which is a web-based application, and the Bionova® Cloud Agent which is a Microsoft™ Windows App that acts as an interface between the Terragene compatible devices and the web-based application.

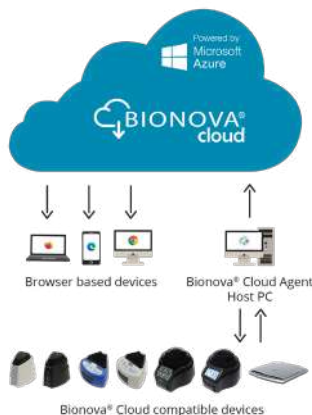

The Bionova® Cloud Traceability Software allows to manage and store the readout results of Self-Contained Biological

⤵ Bionova® Cloud Environment

Indicators and Hygiene Monitoring System Indicators in a secure and user-friendly way.

The Bionova® Cloud Traceability Software allows matching the information of an Indicator result with the sterilizer or washing machine used, the operator, cycle characteristics, and all relevant information for allowing each institution achieve reliable documentation compliance and safe-keeping.

The Bionova® Cloud Agent handles all communications with Terragene® compatible electronic devices and the Host PC where the Agent App runs.

Bionova® Cloud Agent then acts as an interface between the Terragene compatible devices and the Bionova® Cloud Traceability software and sends the information generated from the devices to the Microsoft™ Azure powered Cloud server where the Traceability Software Web App runs and stores the information.

The user can then access to the information saved to the Cloud via any device with a compatible web browser.

To access to the Bionova® Cloud Environment please visit www.terragene.com/bionova-cloud.

Threshold Mode selection for PRO1 Indicators

The Bionova® Cloud Environment allows the selection of the Protein Quantification Threshold Mode and Threshold values throughout its web interface.

Note: Threshold Mode selection is only available for the latest firmware versions. Update your auto-reader's firmware before carrying out any of the steps below. Please refer to the Firmware update section for more information.

- 1|Connect your auto-reader to a PC where Bionova® Cloud Agent is installed.
- 2|Run and Log-in to the Bionova® Cloud Agent. Wait until the Agent lists the incubator.
- 3|Access as the Administrator user to the Bionova® Cloud Environment Web interface.
- 4|Go to the Configuration > Parameters section tab on the Bionova® Cloud Web Interface left side menu.
- 5|Select the Threshold working mode for your auto-reader: HTM 01-01 or ISO 15883-5. Save the selected mode clicking on the SAVE button.
- 6|Select the Threshold values for the selected mode. Save the selected Threshold values by clicking on the SAVE button.

Note: If the process is carried out successfully your auto-reader will print a ticket detailing the Threshold Mode selected.

ISO 15883-5 Threshold Mode

Note: This mode is only valid for the Chemdye® PRO1 MICRO.

The new ISO 15883-5:2021 Standard implements new recommendations for taking action based on the findings of hygiene monitoring indicators. One of the major features of this revision of the standard is that the protein quantities measured when swabbing an instrument must be related to the swabbing surface in which the sample was taken for correct decision making over decontamination and washing equipment.

To obtain an estimation of the swabbing surface area, the new Bionova® Cloud Surface Eye Mobile App was designed. The Surface Eye Mobile App is a new proprietary application developed by Terragene compatible with Android OS that allows the user to obtain an estimation of an instrument's swabbed surface using complex machine learning technologies in a few simple steps. The App also implements seamlessly integration with the Bionova® Cloud Environment.

Linking protein quantification readout data (in µg) informed by an auto-reader, and swabbing surface data (in cm2) informed by the Surface Eye App, throughout the Bionova® Cloud Environment allows the creation of ratios of protein quantities and swabbing surface area (in µg/cm2) that can be compared with ISO 15883-5:2021 style thresholds.

ISO 15883-5 Workflow

Note: This workflow is only valid for the Chemdye® PRO1 MICRO.

Take the following steps for linking protein quantification readout data and swabbing surface data through the Bionova® Cloud Environment.

A) Set-up

1|Set-up your auto-reader for ISO 15883-5 Threshold Mode. Please refer to the *Threshold Mode selection on Bionova® Cloud Environment* section for more information.

2|Download the Bionova® Cloud Surface Eye APP from Google Play Store on your Android compatible device.

Note: Make sure your Android device has a working camera for the Surface Eye App to work as intended.

B) Login and authentication

1|Log-in to the Bionova® Cloud Agent on the PC connected to your Bionova® MiniPro Auto-reader.

2|Log-in to the Bionova® Cloud Surface Eye APP with the same credentials used on the Bionova® Cloud Agent.

3|Log-in to the Bionova® Cloud Web Interface with the same

↳ Bionova® Cloud Environment

credentials used on the Bionova® Cloud Agent.

C) Swabbing and surface estimation

- 1| Set the instrument to be swabbed over the Surface Eye Card. Please keep in mind that the swabbing area must be fully contained on the card for the Surface Eye APP to properly estimate the swabbing surface area.
- 2| Tap on the icon, and align the 3 position markers from your phone screen with the 3 position markings on the Surface Eye card. Once the position markers are aligned, the App will take a photo automatically.
- 3| Select the area of the instrument to be swabbed and tap on the icon.
- 4| The APP will automatically select and estimate the surface (cm²) of the selected swabbing area.

It is a good practice to standardize the swabbing area for each instrument. Defining and using the same swabbing area for a given instrument allows the sampling process to be repeatable through time and deliver valuable statistical information.

Note: According to ISO 15883-5:2021 Standard, the recommended values for the Alert and Action threshold are 3 µg/cm² and 6.4 µg/cm², respectively. As both ratios relate protein quantity of a sample to the swabbing surface from which the sample is taken, please make sure to use standardized surfaces on the range of 1 to 7 cm². The use of higher swabbing surfaces (>7.6 cm²) imply that the protein quantity to define the action threshold would be above the 50 µg of the PRO1 Hygiene Monitoring System quantization range and thus cannot be properly used.

- 5| Define an instrument code and a description to fully identify the swabbing area and the surface acquisition details.

Note: Choose a descriptive code and description for the instrument so it is easier to link the surface data with the protein readout information later on the Bionova® Cloud Environment.

- 6| Check the *Both sides* check-box if you plan to swab both sides of the instrument. Checking the button will duplicate the selected swabbing area to account for the double sided swabbing procedure.
- 7| Once ready, tap the icon. The APP will upload all the surface information to your Bionova® Cloud Environment account.
- 8| The surface acquisition details can be edited from the Apps' home menu swiping the instrument code to the left.

D) PRO1 Indicator incubation and readout

- 1| Follow the instructions for use of your PRO1 Indicator to take a protein sample of the selected instrument.

Note: Make sure to swab evenly the same surface area that was selected on the Surface Eye App.

Note: Make sure you swab both sides of the instrument if the Both sides check-box was selected on the Surface Eye APP.

- 2| Carry out the incubation and readout of the PRO1 Indicator as described on the Instructions for Use section of this manual. Wait for a readout result to be informed.

E) Linking protein readout information and swabbing surface information

- 1| Once the readout result is informed by the auto-reader. Go to the *Hygiene Monitoring > Finished* tab on the Bionova® Cloud Web Interface right side menu and fill in the PRO1 Indicator readout information.

- 2| Click on the *Assign Area* button and select the surface acquisition data details of the swabbed surface.

Note: Make sure the surface acquisition information corresponds to the protein readout data so that the correct ratios can be obtained. To check if the surface information is the correct one, click on the magnifying glass to view the swabbing surface image saved on the Bionova® Cloud environment.

- 3| Click the Confirm button to save the details, or the *Confirm and move to saved* button to save the details and move the readout to the Bionova® Cloud Database accessible through *Dashboard > Saved* section tab on the Bionova® Cloud Web Interface left side menu.

Bionova® Cloud Surface Eye Mobile App advanced features

Note: The Surface Eye Mobile App is only compatible with the ChemDye® PRO1 MICRO.

Redefining the swabbing area of an instrument

You can redefine a previously saved surface area of an instrument on the Surface Eye app, and take a new photo to assign a new swabbing area to the instrument. For this swipe left on the instrument code, and tap the icon. Take a new photo and select the new swabbing area.

Editing an instrument code and description

You can edit the details of any of the instrument codes previously saved on the Surface Eye app. For this swipe left on the instrument code, and tap the icon.

Conversion of ISO 15883-5 thresholds

Once a swabbing surface area has been saved and assigned to an instrument on the Surface Eye App, the details of the surface can be accessed by typing the instrument code.

On the details screen, the Alert and Action Thresholds (in µg/cm²) as defined on the Bionova® Cloud Environment, are converted and shown to the user as protein quantity thresholds

⬇ **Bionova® Cloud Environment**

(µg) for the selected surface.

This allows for direct visual comparison between the protein quantity found on the sample as informed on the auto-reader printed ticket, and the protein quantities that correspond to the alert and action thresholds for the defined swabbing area.

■ **Cleaning and maintenance**

Cleaning and decontamination of external surfaces

Disconnect the power supply cable and the USB cable from the auto-reader. If the device is hot, wait until it has cooled down before handling it.

Clean the external surfaces of the device using a microfiber cloth moistened with a solution of mild dish washing detergent and water. Wring out the cloth so it is damp but not dripping before cleaning and wiping the outer surfaces of the auto-reader. Then, moisten a clean microfiber cloth with just water, and repeat the procedure until all traces of detergent are removed from the external surfaces of the device. After cleaning, allow the auto-reader to air dry for at least 1 hour before connecting the power supply cable or the USB cable again.

This cleaning procedure can be followed whenever considered appropriate.

This cleaning procedure must be followed each time a spill occurs on any of the external surfaces of the auto-reader.

If further cleaning is required, or if you have doubts about the cleaning agents you may use, please contact your local distributor.

Note: Do not clean the internal parts of the device.

Note: Do not pour liquid onto the device or immerse it in any liquid. Do not allow any liquid to enter the device while it is being cleaned.

Maintenance

The Bionova® MiniPro Auto-reader does not require routine maintenance.

■ **Troubleshooting**

Problem: *The auto-reader does not start.*

Possible causes: The power supply is not connected.

Actions: Check that the power supply is connected to

the mains. Check that the DC plug of the power supply is connected to the rear of the auto-reader.

Problem: *The auto-reader informs an error in an incubation position during "auto-test".*

Possible causes: An indicator is placed in the incubation position during the auto-test.

Dust particles might be obstructing the readout mechanism.

Actions: Check that every incubation position is empty during the auto-test. Restart the device.

If after restarting the device the problem persists, use air to remove any dust inside a position. Do not insert solid objects. Once cleared, restart the auto-reader.

Note: Do not use the auto-reader in dusty environments.

Problem: *An incubation cannot be run in an incubation position (position's Red LED Indicator is on).*

Possible causes: Position disabled. Error in that position during the "auto-test".

Actions: Make sure that the position is empty when starting the auto-reader. Once cleared, restart the auto-reader.

Problem: *The auto-reader does not run an incubation in any position.*

Possible causes: The incubation temperature is not stable.

Actions: Wait until temperature is stable before any incubations.

Problem: *It is not possible to change temperature and/or time setting.*

Possible causes: There is an ongoing reading.

Actions: Wait for any incubation to complete and try again.

Problem: *It is not possible to start a Chemdye® PRO1 indicator incubation (Pen not valid ticket).*

Possible causes: The protein pen condition is not appropriate for its incubation.

Actions: Make sure that the solution on the reading cone is sufficient. Make sure the indicator solution is not overly saturated or already changing its color (i.e., not green).

Do not incubate an indicator twice. Please follow the Instructions for Use before its incubation.

Problem: *The auto-reader does not detect the protein Pen (Pen not detected ticket).*

Possible causes: Protein pen is not correctly placed in the incubation position.

Actions: Make sure the indicator is fully placed at the bottom of the incubation position before its incubation.

Problem: *The printer does not print (Blue attention light blinks quickly).*

Possible causes: The printer cover is not tightly closed.

Printer without paper.

Actions: Check that the cover is tightly closed. Place a new

↩ Troubleshooting

paper roll in the right direction.

Problem: *The printer releases unprinted paper.*

Possible causes: Paper roll is not placed correctly.

Actions: Place the paper according to the directions on the *Replacement of the paper roll section*.

Problem: *The auto-reader will not update.*

Possible causes: Bionova® Bioupdate (Firmware updater utility) is not running.

Actions: Install and run Bionova® Bioupdate and follow the instructions on the *Firmware update section*.

Problem: *The auto-reader is not detected by Bionova® Cloud Agent.*

Possible causes: The auto-reader is turned off.
The auto-reader is not connected to the PC.

Actions: Follow the directions on the Start-up section to set-up the device properly.

■ Warranty

The products are guaranteed to be free from material and workmanship defects when properly installed, maintained and used for their intended purpose as indicated in the applicable product label and/or the User Guide. The warranty only applies to the original purchaser.

Term

The warranty period for the Bionova® MiniPro Auto-reader is 1 (one) year from the date of installation and may never be extended beyond 5 (five) years from the product's date of manufacture.

Limitation of liability

Terragene S.A. shall not be held liable for any loss or damage that result from the unsuitable use of the equipment, negligence, or user's full responsibility.

Technical assistance

Terragene S.A.
Ruta Nacional N° 9, KM 280 - CP 2130.
Parque Industrial Micropi - Alvear - Santa Fe - Argentina.

